

HYCISUN[®]

REF HS0501A

FFP2 Maske / FFP2 Mask

Persönliche Schutzmaske

MICRO-MEDICAL



CE 2797

EN 149: 2001 + A1: 2009

CARTON DIMENSION (FFP2 - White - 20er)

HYCISUN®

1 PC/OPP

20 PCS/box

1000 PCS/carton

20000 PCS/pallet

EAN: 4260676530003

CE 2797



MICRO-MEDICAL

FFP2-MASKE

PERSÖNLICHE SCHUTZMASKE EN149:2001+A1:2009

Faltbare Partikel -Atemschutzmaske

Hohe Filtrationseffizienz
Geringer Atemwiderstand
Bequem zu tragen



HYGISUN[®]

REF HS0501A

20 Stück

Einmalgebrauch

CE 2797

20 Stück

Einmalgebrauch

CE 2797

MICRO-MEDICAL

Bedienungsanleitung Fitting instructions



Nehmen Sie die Maske an den Ohrschlaufen in die Hand und drücken Sie diese mit dem Bügel auf den Nasenrücken gegen Ihr Gesicht, während Sie die Ohrschlaufen hinter Ihren Ohren positionieren.

Take the mask by the ear loops in your hand and press it against your face with the strap on the bridge of your nose while you position the ear loops behind your ears.



Formen Sie den Bügel mit beiden Händen in die Form Ihrer Nase.
Shape the nose clip into the shape of your nose with both hands.



Testen Sie die Passform. Nehmen Sie beide Hände über die Atemschutzmaske und atmen Sie kräftig aus. Wenn Luft um Ihre Nase strömt, ziehen Sie den Bügel fester.

Test the correct fit. Put both hands over the respirator and exhale forcefully. When air flows out around your nose, press the nose clip tighter.

HINWEIS ZUR VERWENDUNG: / NOTICE FOR USE:

- Bitte verwenden Sie dieses Produkt nicht in der Nähe einer Feuerquelle.
Please do not use this product near fire sources.
- Da es sich bei diesem Produkt um eine Einwegmaske handelt, kann es nicht durch Waschen wiederverwendet werden.
As this product is a disposable mask, it cannot be reused through washing.
- Von hohen Temperaturen und Luftfeuchtigkeit fernhalten und an einem sauberen Ort aufbewahren.
Keep it away from high temperature and humidity and keep it in clean place.
- Persönliche Schutzmaske, Nicht medizinisch.
personal protective mask, non medical.
- Verwenden Sie einzeln verpackte Produkte, sobald diese ausgepackt sind.
Use individually packaged products as soon as they are unpacked.

MICRO-MEDICAL

FFP2-MASK

PERSONAL PROTECTIVE MASK EN149:2001+A1:2009

Foldable Particulate Respirator

High filtration efficiency
Low respiratory resistance
More comfortable to wear

20PCS

Single Use



CE 2797

HYCISUN[®]

REF H50501A

FFP2 Mask

EN149:2001+A1:2009

170mm (6.7") x 95mm (3.7")

1.5mm (0.06")

1.5mm (0.06")

1.5mm (0.06")

1.5mm (0.06")

1.5mm (0.06")

1.5mm (0.06")

1.5mm (0.06")

1.5mm (0.06")

1.5mm (0.06")

1.5mm (0.06")

1.5mm (0.06")

1.5mm (0.06")

1.5mm (0.06")

1.5mm (0.06")

20PCS

Single Use




CE 2797

MICRO-MEDICAL

FFP2 Maske

EN149:2001+A1:2009

 **WICHTIG:** Die Atemschutzmaske FFP2 bietet Schutz vor Pollen, Viren und Industriestaub.

 **IMPORTANT:** The respiratory protection mask FFP2 is designed to protect from pollen, virus and industrial dust.

ANWENDUNG: / APPLICATION:

Die Maske wird in der Schutzindustrie bei Staubbemittlung, während des Baus zur Staubverhütung, beim Metallguss, Steinabbau, in der Elektronik, Pharmazie, der physikalischen Verarbeitung und beim Schweißen verwendet und bietet einen guten Schutz gegen Sandstürme, Dunst und PM2.5. Kann wirksam vor Pollenallergien, Virusübertragung usw. schützen.

It is used in the industry for dust generation during construction, dust prevention, metal casting, stone mining, electronics, pharmaceutical, physical processing and grinding. It also offers good protection against sandstorms, haze and PM2.5. Can effectively protect pollen allergy, virus transmission, etc.

VERFALLSDATUM: / EXPIRATION DATE:

Lagertemperatur: -20 ~ -38 °C, Lagerfeuchtigkeit ≤ 80%, Haltbarkeit: 2 Jahre in trockenen Innenräumen.

The storage temperature is -20 ~ -38 °C, the storage is moderate ≤ 80%, The validity period is 2 year in the dry indoor environment.



Hunan Dreaming Cloud E-Commerce CO., Ltd
Block 1, Smart Tech Park, 57# Huangxing Avenue, Changsha Economic and Technological Development Zone, Changsha, Hunan, China

EC REP

Sunbeam International GmbH
Schumacherstr. 12, 52146 Würselen, Germany

PZN: 16865038



4 260676 530003

MICRO-MEDICAL

HYCISUN[®]
FFP2 Maske
Nicht medizinisch EN149:2001+A1:2009

FFP2-MASKE
Nicht medizinisch EN149:2001+A1:2009

**Faltbare Partikel-
-Atemschutzmaske**
Hohe Filtrationseffizienz
Geringer Atemwiderstand
Bequem zu tragen

20 Stück



HYCISUN[®]
REF HS0501A

MICRO-MEDICAL



LOT:20201025-01-A
PD:2020/10/25
MHD/BBD:2022/10/24

20 pcs

Single Use

High filtration efficiency
Low respiratory resistance
More comfortable to wear

FFP2-MASK
PERSONAL PROTECTIVE MASK EN149:2001-AT:2008
Foldable Particulate Respirator

HYCISIN
L. INC. / M. S. S. O. I. A.

CE 2797

MICRO-MEDICAL



Persönliche Schutzmaske

PERSONAL PROTECTIVE MASK

1 Stück / Piece

1 ШТУК / ПЬЕСА

MICRO-MEDICAL

ПЕРСОНАЛЬНАЯ ПРОТЕКТИВНАЯ МАСКА



Persönliche Schutzmaske

PERSONAL PROTECTIVE MASK

1 Stück/ Piece

1 Stück/ Piece

MICRO-MEDICAL

HYCISUN

QUALIFIED CERTIFICATE

产品名称 FFP2个人防护口罩(不作为医疗防护使用)
Product Name FFP2 personal protective mask.(For personal protective only)
执行标准 EN149:2001 + A1:2009
Standard EN149:2001 + A1:2009
产品规格 16×10.5厘米
Product Size 16×10.5CM
材质 30%熔喷布+70%无纺布
Material 30% MELT-BLOWN FABRIC+70% NONWOVEN FABRIC

质检员

Checker

生产日期

Date

生产批号

Lot code

使用周期 一次性

Useage count

有效期 2年

Period of validity 2 years

生产企业 湖南云想生活电子商务有限公司

Manufacturer Hunan Dreaming Cloud E-Commerce CO., Ltd

生产地址 长沙经济技术开发区黄兴大道南段
57号星为创芯园1栋501号

Address

Block 1, Smart Tech Park, 57# Huangxing Avenue, Changsha,
Economic and Technological Development Zone, Changsha,
Hunan, China

储存条件: 本品应储存温度-20~38°C, 储存湿度≤80%
避光干燥的室内环境下, 通风良好, 无腐蚀性气体的清洁
环境中, 如贮存不当导致发霉变质禁用。

STORAGE CONDITIONS AND METHODS: The storage temperature is -20~38°C, and
the relative humidity is not more than 80%. Well ventilated and clean environment
without corrosives, please do not use if the product gets mildewed or
deteriorated due to improper storage.

本产品为个人防护用品, 不作为医疗防护使用

THIS PRODUCT IS UNDER PERSONAL PROTECTIVE EQUIPMENT DIRECTIVE
(PEE)FOR PERSONAL PROTECTIVE ONLY

MADE IN CHINA



WVDE IM CHINA

WVDE IM CHINA
WVDE IM CHINA
WVDE IM CHINA

MICRO-MEDICAL

ANLEITUNG**Norm:**

Dieses Produkt entspricht der Norm EN149:2001 + A1:2009 für Atemschutzgeräte – Halbmaske zur Filterung zum Schutz vor Partikeln. Diese Filtermasken sind gemäß der Verordnung der Europäischen Kommission (EU) 2016/425 über PSA als Persönliche Schutzausrüstung in der Kategorie III eingestuft und entsprechend gekennzeichnet

Bestimmungsgemäße Verwendung:

Die Staubmaske ist als Kategorie FFP 2 eingestuft. Sie schützt vor Partikeln, Nebel, Rauch und Aerosolen auf Ölbasis. Die Verpackung schützt die Maske vor der Verwendung. Schützt wirksam vor Pollen. Die Maske kann nur zum persönlichen Schutz verwendet werden, nicht für medizinische Zwecke. Maske nicht bei der Brandbekämpfung und in explosionsgefährdeten Bereichen nutzen.

Dichtstztest

1. Bedecken Sie die Maske vorsichtig mit beiden Händen ohne den Dichtstz zu verändern.
2. stark Ausatmen.
3. Bei einer Leckage im Nasenbereich, den Nasenbügel neu anpassen. Dichtstzprüfung wiederholen.
4. Bei einer Leckage am Maskenrand, den Sitz der Bänder überprüfen und anpassen. Dichtstzprüfung wiederholen.

Wenn Sie KEINEN richtigen Dichtstz erreichen können, betreten Sie NICHT den Gefahrenbereich. Informieren Sie Ihren Vorgesetzten.

Warnungen und Einschränkungen:

- Vergewissern Sie sich immer, dass das Produkt:
 - Geeignet ist für die Anwendung;
 - Korrekt angelegt ist;
 - Während des gesamten Aufenthalts im Gefahrenbereich getragen wird;
 - Ersetzt wird, wenn notwendig.
- Richtige Auswahl, Schulung, Gebrauch und gegebenenfalls Reinigung sind die Voraussetzungen dafür, dass das Produkt den Anwender vor bestimmten luftgetragenen Gefahrstoffen schützt.
- Die Nichtbefolgung aller Anweisungen zur Anwendung der Maske und/oder die Fehlbenutzung während des Aufenthaltes im Gefahrenbereich kann die Gesundheit des Anwenders beeinträchtigen und zu schweren Erkrankungen oder Dauerschäden führen.
- Beachten Sie bei der Auswahl und richtigen Anwendung nationale Bestimmungen und alle mitgelieferten Informationen.
- Vor Gebrauch muss der Anwender, in Übereinstimmung mit den nationalen Regeln, in der funktionsgerechten Handhabung geschult sein.
- Dieses Produkt schützt nicht vor Gasen und Dämpfen.
- Verwenden Sie die Maske nicht in Umgebungen mit weniger als 19,5% Sauerstoff
- Verwenden Sie die Masken nicht in Umgebungen mit unbekanntem Gefahrstoffen oder Konzentrationen, die die zulässigen Höchstwerte übersteigen.
- Verwenden Sie die Maske nicht, wenn Gesichtshaare im Bereich des Dichtrandes einen korrekten Dichtstz der Maske verhindern.
- Verlassen Sie sofort den belasteten Bereich, wenn:
 - a) Das Atmen schwer fällt.
 - b) Schwindel oder andere Beschwerden auftreten.
 - c) Die Maske beschädigt wird.
 - d) Geruch oder Geschmack des Gefahrstoffs oder eine Reizung auftritt.
- Entsorgen und ersetzen Sie die Maske, wenn sie beschädigt ist, der Atemwiderstand stark erhöht ist oder am Ende einer Schicht.
- Die Maske darf niemals verändert oder repariert werden.
- Die Maske ist zum einmaligen Gebrauch vorgesehen und ist danach entsprechend der nationalen Vorgaben zu entsorgen.


Transport und Lagerung:

Die Partikelmasken haben eine Lagerdauer von 2 Jahren. Das Ende der Lagerdauer ist auf der Verpackung angegeben. Vergewissern Sie sich vor Gebrauch immer, dass das Produkt noch innerhalb der Lagerdauer liegt. Das Produkt sollte sauber, trocken und im Temperaturbereich von -20°C bis +30°C bei einer maximalen rel. Luftfeuchtigkeit von 80% gelagert werden. Für Lagerung und Transport die Originalverpackung verwenden. Nicht direkter Sonnenstrahlung aussetzen.


6pcs

Mask Mate - Belt Extension Kit


Put the belt across the semi-sealed hook, then put the opposite belt to match your head size



Instruction Image



type I



type II



type III

Instruction Image



type III



type II

MICRO-MEDICAL



HYUNDAI
HS0501A FFP2 NR
EN149:2001+A1:2009
CE 2137

MICRO-MEDICAL

取得国外标准认证或注册的非医用口罩生产企业清单

Name List of Non-Medical Use Face Masks Companies with

序号 No.	生产企业 Company	统一社会信用代码 Uniform Social Credit Code	国外注册认证情况 Status of Certification / Authorization in Other Countires
377	洛阳科利达科技有限公司 Luoyang Kelida Technology Co., Ltd.	91410306MA44H8X31L	German Mask: EURL
378	仙桃市平路欣生设备有限公司 Xiانتو Qiantong Life Saving Equipment Co., Ltd.	91429081MA4F9AHL5P	CE
379	湖南云想生活电子商务有限公司 Hunan Dreaming Cloud E-Commerce CO., Ltd	91430105MA4LAAUW8C	CE
380	连云港美琪医疗用品有限公司 Lianyungang Meiqi Medical Supplies Co., Ltd.	91320734566800367E	CE
381	南京海思医疗器械有限公司 Nanjing Hoosy Medical Apparatus and Instruments Co., Ltd.	91320133MA209F20048	CE
382	江苏嘉盛服饰有限公司 Jiangsu Jiasheng Clothing Co., Ltd	91320921MA1N90UE28	CE

EU-KONFORMITÄTSERKLÄRUNG

Diese Konformitätserklärung wurde unter der alleinigen Verantwortung des Herstellers

Hunan Dreaming Cloud E-Commerce CO., Ltd.

Block 1, Smart Tech Park, 57 # Huangxing Avenue, Changsha Economic and Technological Development Zone, Changsha, Hunan, China

ausgestellt.

EG-Vertreter: Sunbeam International GmbH, Schumanstr.12, Würselen 52146 Deutschland

Hiermit wird erklärt, dass die folgende persönliche Schutzausrüstung (PSA)

Produktbeschreibung: HYGISUN Partikelfilter-Halbmaske

Produktmodell (e): HS0501A FFP2 NR ohne Ventil

den Bestimmungen der folgenden europäischen Verordnung entspricht:

PSA-Verordnung (Persönliche Schutzausrüstung)

Das Modell entspricht den Bestimmungen der Verordnung (EU) 2016/425, PSA zur Verwendung durch Angehörige der Gesundheitsberufe gemäß der Empfehlung der Kommission 2020/403 und der Nationalen Norm zur Umsetzung der harmonisierten europäischen Normnummer (n):

EN 149: 2001 + A1: 2009

und ist identisch mit der PSA, die Gegenstand einer EU-Typprüfung ist (Modul B der Verordnung (EU) 2016/425), auf die auf der Zertifikatsnummer verwiesen wird:

Zertifikat Nr.: CE 750475 (Ausstellungsdatum: 09/06/2021)

herausgegeben von BSI Group Niederlande BV

John M. Keynesplein 9, 1066 EP, Amsterdam, Niederlande (Notified Body No. 2797)

und entspricht den Verfahren in Modul C2 der Verordnung (EU) 2016/425 unter der Überwachung der BSI Group The Netherlands BV (Notified Body Nr. 2797), auf die auf dem vom BSI ausgestelltem Zertifikat CE 750476 (Ausstellungsdatum: 09/06/2021) verwiesen wird.

Changsha, China, 10.06.2021

OuYang Zhouya

OuYang Zhouya

(Nachname Name)

Qualitätsmanager

Hunan Dreaming Cloud E-Commerce CO., Ltd.



EU Type Examination Certificate

This is to certify that:

Sunbeam International GmbH
Schumanstr. 12
Würselen
52146
Germany

Holds Certificate Number:


CE 750475

In respect of:

**Respiratory protective devices - Filtering half masks to protect against particles -
To EN 149:2001+A1:2009
Model: HYGISUN HS0501A.**

on the basis that BSI carried out the relevant Type Examination procedures under the requirements with the Regulation (EU) 2016/425 of the European Parliament and Council relating to Personal Protective Equipment Regulation (PPE) Annex V (Module B) and meets the relevant health and safety requirements specified in Annex II

For and on behalf of BSI, a Notified
Body for the above Regulation
(Notified Body Number 2797):

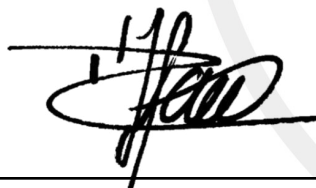

Drs. Dave Hagenaaars, Managing Director

First Issued: 2021-06-09

Latest Issue: 2021-06-09

Effective Date: 2021-06-09

Expiry Date: 2026-06-09

Page: 1 of 3



...making excellence a habit.™

EU Type Examination Certificate

No. CE 750475

Product Specification

Product Type: Filtering half masks to protect against particles.

Model: HYGISUN HS0501A.

Product description: The particulate respirator is designed to protect against solid and non-volatile liquid particles.

The masks are a single size, non-sterile, non-valved product held on the face by a pair of elasticated ear loops.

The masks are intended for single shift use as denoted by the classification symbol NR.

Technical specification: EN 149:2001+A1:2009 – Respiratory Protective Devices - Filtering half masks to protect against particles.

EN 149 classification: FFP2 NR.

First Issued: 2021-06-09

Latest Issue: 2021-06-09

Effective Date: 2021-06-09

Expiry Date: 2026-06-09

Page: 2 of 3

This certificate has been issued by and remains the property of BSI Group The Netherlands B.V., John M. Keynesplein 9, 1066 EP Amsterdam, The Netherlands and should be returned immediately upon request.
To check its validity telephone +31 20 3460780. An electronic certificate can be authenticated [online](#).

BSI Group The Netherlands B.V., registered in the Netherlands under number 33264284, at John M. Keynesplein 9, 1066 EP Amsterdam, The Netherlands
A member of BSI Group of Companies.

EU Type Examination Certificate

No. CE 750475

Certificate Administration Details

Technical File reference: TCF.02.

Certificate Amendment Record:

Issue date	Comments	BSI Review Number
June 2021	First issue under PPE Regulation (EU) 2016/425. Product initially Certified as a "Covid-19" mask by BSI, Certificate CE 730303 refers.	2797:2021:3339407

Certificate validity

The Certificate holder is responsible for ensuring that the Notified Body is advised of changes to any aspect of the overall processes utilised in the manufacture of the product, failure to do so could invalidate the Certificate in respect of product manufactured following the introduction of such changes.

The validity of the Certificate for the products is also dependent on the maintenance of the EU Conformity to Type based on Internal Production Control plus supervised product checks at random intervals, Annex VII (Module C2) as referenced on BSI issued Certificate CE 750476.

First Issued: 2021-06-09

Latest Issue: 2021-06-09

Effective Date: 2021-06-09

Expiry Date: 2026-06-09

Page: 3 of 3

This certificate has been issued by and remains the property of BSI Group The Netherlands B.V., John M. Keynesplein 9, 1066 EP Amsterdam, The Netherlands and should be returned immediately upon request.
To check its validity telephone +31 20 3460780. An electronic certificate can be authenticated [online](#).

BSI Group The Netherlands B.V., registered in the Netherlands under number 33264284, at John M. Keynesplein 9, 1066 EP Amsterdam, The Netherlands
A member of BSI Group of Companies.

Conformity to Type based on Internal Production Control plus supervised product checks at random intervals

This is to certify that:

Sunbeam International GmbH
Schumanstr. 12
Würselen
52146
Germany

Holds Certificate Number:


CE 750476

In respect of:

**For the manufacture of respiratory protective devices -
Filtering half masks to protect against particles - To EN 149:2001+A1:2009.**

on the basis that BSI carried out the supervised production checks at random intervals under the requirements with the Regulation (EU) 2016/425 of the European Parliament and Council relating to Personal Protective Equipment Regulation (PPE) Annex VII (Module C2)

For and on behalf of BSI, a Notified Body for the above Regulation (Notified Body Number 2797):

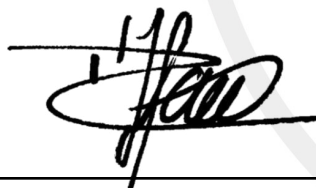

Drs. Dave Hagenaaars, Managing Director

First Issued: 2021-06-09

Latest Issue: 2021-06-09

Effective Date: 2021-06-09

Expiry Date: 2026-06-09

Page: 1 of 2



...making excellence a habit.™

Conformity to Type based on Internal Production Control plus supervised product checks at random intervals

No. CE 750476

Model produced by:

Hunan Dreaming Cloud E-Commerce CO., Ltd
Block 1, Smart Tech Park,
57# Huangxing Avenue,
Changsha Economic and Technological Development Zone,
Changsha,
Hunan,
China

Product details

The respiratory protective device covered by the scope of this Module C2 Certificate and the Technical Specification to which the product is manufactured are as follows:

Product type:	Respiratory protective device – Filtering half masks to protect against particles.
Model:	HYGISUN HS0501A.
Technical Specification:	EN 149:2001+A1:2009 – Respiratory Protective Devices - Filtering half masks to protect against particles.
EN 149 classifications:	FFP2 NR.

Certificate Administration Details:

Certificate Amendment Record:

Issue date	Comments	BSI Review No.
June 2021	First issue. Referenced product initially Certified as a "Covid-19" mask by BSI, with the associated BSI issued Module C2 Certificate CE 730304.	2797:21:3339408

Certificate validity

The Certificate holder is responsible for ensuring that the Notified Body is advised of changes to any aspects of the overall quality system utilized in the manufacture of the products, failure to do so could invalidate the Certificate in respect of product manufactured after the introduction of such changes.

First Issued: 2021-06-09

Effective Date: 2021-06-09

Latest Issue: 2021-06-09

Expiry Date: 2026-06-09

Page: 2 of 2

This certificate has been issued by and remains the property of BSI Group The Netherlands B.V., John M. Keynesplein 9, 1066 EP Amsterdam, The Netherlands and should be returned immediately upon request.
To check its validity telephone +31 20 3460780. An electronic certificate can be authenticated [online](#).

BSI Group The Netherlands B.V., registered in the Netherlands under number 33264284, at John M. Keynesplein 9, 1066 EP Amsterdam, The Netherlands
A member of BSI Group of Companies.


Test Report 3339405.
Sunbeam International GmbH.

Introduction.

This report has been prepared by D. Key and relates to the activity detailed below:

Job/Registration Details		Client Details
Job number:	3339405	Sunbeam International GmbH Schumanstr. 12 Würselen 52146 Germany
Job type:	Testing samples submitted	
Start Date:	17/01/2021	
Test type:	Type	
Sample ID:	10195243	
Registration:	CE 730303	
Scheme:	Negative Pressure RPE	
Protocol:	PP123	
Scheme Manager:	Nathan Shipley	

The report has been approved for issue by T Wicksey – Senior Test Engineer

Approved For Issue	
	Issue Date: 22 March 2021

Objectives.

This is an independent Type Test evaluation to BS EN 149:2001+A1:2009. This report covers the gap testing from the BSI COVID-19 filtering face piece technical specification, for COVID-19 masks for use by healthcare workers. See BSI Test Report 3220780 for the BSI COVID-19 filtering face piece technical specification test results.

Product Scope.

Respiratory protective device- Filtering half masks to protect against particles.

Report Summary.

The samples were received on 18 December 2020 and the testing was started on 17 January 2021.

The samples submitted complied with the requirements of the test work conducted.

Test Samples.

Sample ID	ER Number	Description
1 to 37	10195243	Model: HYGISUN HS0501A FFP2 NR

Description of Test Samples.

Sample Description
Model: HYGISUN HS0501A FFP2 NR. Valveless vertical fold flat particle filtering half mask with elastic earloops and removable plastic earloop clip

Test Requirements.

BS EN 149:2001 + A1:2009

Respiratory protective devices - Filtering half masks to protect against particles.

CLAUSE	REQUIREMENTS	ASSESSMENT
7	Requirements	-
7.1	General	-
7.2	Nominal values and tolerances	-
7.3	Visual Inspection	Pass (1)
7.4	Packaging	N/T (1)
7.5	Material	Pass
7.6	Cleaning and disinfecting	N/A (2)
7.7	Practical performance	N/T (3)
7.8	Finish of parts	Pass
7.9	Leakage	-
7.9.1	Total inward leakage	Pass (3)
7.9.2	Penetration of filter material	Pass (3)
7.10	Compatibility with skin	Pass
7.11	Flammability	Pass
7.12	Carbon dioxide content of inhalation air	N/T (3)
7.13	Head harness	Pass
7.14	Field of vision	Pass
7.15	Exhalation valves	N/A (4)
7.16	Breathing resistance	Pass (3)
7.17	Clogging	N/A (4)
7.18	Demountable parts	N/A (4)
9	Marking	N/T (1)
10	Information to be supplied by the manufacturer	N/T (1)
Appendix A - Test Panel Data		
Product Photographs		

- (1) Packaging, Marking and Information not assessed as requested by BSI Product Certification
- (2) Single use mask
- (3) See also results from BSI COVID-19 filtering face piece technical specification testing, BSI Test Report number 3220780.
- (4) Not a design feature of this product

Glossary of Terms.

Pass: Complies. Tested by BSI engineers at BSI laboratories

Pass 1: Complies. Witnessed by BSI engineers in manufacturers laboratory.

Pass 2: Complies. Tests carried out by third party lab; results accepted by BSI.

Pass*: Report resulted in uncertainty and states that Compliance is more probable than non-compliance.

Fail: Non-compliance. Product does not meet the requirements of this clause.

Fail*: Report resulted in uncertainty and states that Non-compliance is more probable than compliance.

N/T: Not Tested

N/A: Not Applicable

AR: As Received

TC: Temperature Conditioned

SW: Simulated Wear

FT: Flow Tested

MS: Mechanical strength

MMDF: Manufacturer's Minimum Design Flow

Conditions of Issue.

This Test Report is issued subject to the conditions stated in current issue of 'BSI Terms of Service'. The results contained herein apply only to the particular sample(s) tested and to the specific tests carried out, as detailed in this Test Report. The issuing of this Test Report does not indicate any measure of Approval, Certification, Supervision, Control or Surveillance by BSI of any product. No extract, abridgement or abstraction from a Test Report may be published or used to advertise a product without the written consent of BSI, who reserve the absolute right to agree or reject all or any of the details of any items or publicity for which consent may be sought.

Should you wish to speak with BSI in relation to this report, please contact Customer Services on +44 (0)8450 80 9000.

BSI
Kitemark House
Maylands Avenue
Hemel Hempstead
Hertfordshire
HP2 4SQ



0135

Opinions and Interpretations expressed herein are outside the scope of our UKAS accreditation.

Unless otherwise stated, any results not obtained from testing in a BSI laboratory are outside the scope of our UKAS accreditation.

Test Results.

BS EN 149:2001 + A1:2009

Respiratory protective devices - Filtering half masks to protect against particles.

CLAUSE	REQUIREMENTS	ASSESSMENT
7.1	General In all tests all samples shall meet the requirements.	-
7.2	Nominal values and tolerances Unless otherwise specified, the values stated in this European Standard are expressed as nominal values. Except for temperature limits, values, which are not stated as maxima or minima, shall be subject to a tolerance of $\pm 5\%$. Unless otherwise specified, the ambient temperature for testing shall be (16 – 32) °C, and the temperature limits shall be subject to an accuracy of $\pm 1^\circ\text{C}$.	-
7.3	Visual Inspection The visual inspection shall also include the marking and the information supplied by the manufacturer.	Pass (1)
7.5	Material Materials used shall be suitable to withstand handling and wear over the period for which the particle filtering half mask is designed to be used. After undergoing the conditioning described in clause 8.3.1 of the standard none of the particle filtering half masks shall have suffered mechanical failure of the facepiece or straps. Three particle filtering half masks shall be tested. When conditioned in accordance with 8.3.1 and 8.3.2 the particle filtering half mask shall not collapse. Any material from the filter media released by the air flow through the filter shall not constitute a hazard or nuisance for the wearer. Testing shall be done in accordance with 8.2.	Pass Pass Pass
7.8	Finish of parts Parts of the device likely to come into contact with the wearer shall have no sharp edges or burrs. Testing shall be done in accordance with 8.2.	Pass

(1) Marking and user information were not assessed as requested by BSI Product Certification

Test Results. (Continued)

CLAUSE	REQUIREMENTS	ASSESSMENT
--------	--------------	------------

7.9 Leakage

7.9.1 Total inward leakage

The laboratory tests shall indicate that the particle filtering half mask can be used by the wearer to protect with high probability against the potential hazard to be expected.

Pass (1)
See Table A

The total inward leakage consists of three components: face seal leakage, exhalation valve leakage (if exhalation valve fitted) and filter penetration.

For particle filtering half masks fitted in accordance with the manufacturer's information, at least 46 out of the 50 individual exercise results (i.e. 10 subjects x 5 exercises) for total inward leakage shall be not greater than

- 25% for FFP1
- 11% for FFP2
- 5% for FFP3

and, in addition, at least 8 out of the 10 individual wearer arithmetic means for the total inward leakage shall be not greater than

- 22% for FFP1
- 8% for FFP2
- 2% for FFP3

Testing shall be done in accordance with 8.5.

Table A: Clause 7.9.1 - Total inward leakage.

Test candidate	Sample	Pre-test condition	Inward leakage (%).					Average
			A	B	C	D	E	
			Walking	Walking with head side to side	Walking with head up & down	Walking and talking	Walking	
LM2	8	TC	7.2973	3.9167	5.7087	3.2365	5.1736	5.0666
SI1	9	TC	0.2104	0.2047	0.2353	0.2276	0.1237	0.2003
KH1	10	TC	0.2112	0.2296	0.2503	0.5231	0.6973	0.3823
CB1	11	TC	3.0178	1.8510	8.0745	1.8897	5.6798	4.1025
JW1 (2)	12	TC	0.5893	0.9512	0.7366	0.4300	0.6535	0.6721

- (1) Results for the remaining 'as received' samples are covered in BSI Test Report number 3220780 for the BSI COVID-19 filtering face piece technical specification testing.
- (2) Earloop clip used.

Test Results. (Continued)

CLAUSE	REQUIREMENTS	ASSESSMENT
7.9.2	<p>Penetration of filter material</p> <p>The penetration of the filter of the particle filtering half mask shall meet the requirements of Table 1</p> <p>A total of 9 samples of particle filtering half masks shall be tested for each aerosol. Testing in accordance with 8.11 using the Penetration test according to EN 13274-7, shall be performed on:</p> <ul style="list-style-type: none"> 3 samples as received, 3 samples after the simulated wearing treatment described in 8.3.1. <p>Testing in accordance with 8.11 using the Exposure test with a specified mass of test aerosol of 120 mg, and for particle filtering devices claimed to be re-usable additionally the Storage test, according to EN 13274-7, shall be performed:</p> <p>for non-re-usable devices on:</p> <ul style="list-style-type: none"> 3 samples after the test for mechanical strength in accordance with 8.3.3 followed by temperature conditioning in accordance with 8.3.2. <p>for re-usable devices on:</p> <ul style="list-style-type: none"> 3 samples after the test for mechanical strength in accordance with 8.3.3 followed by temperature conditioning in accordance with 8.3.2 and followed by one cleaning and disinfecting cycle according to the manufacturer's instruction. 	<p>Pass (1) See Tables B and C</p> <p>Pass (1) See Table D and E</p> <p>N/A (2)</p>

Table B: Clause 8.11 - Sodium Chloride penetration test.

Sample	Pre-test condition	Continuous flow (l/min)	Penetration (%)	
			Limit	Measured
16	SW	95	6.0	0.1635
17	SW	95	6.0	0.1645
18	SW	95	6.0	0.1542

Table C: Clause 8.11 - Paraffin oil penetration test.

Sample	Pre-test condition	Continuous flow (l/min)	Penetration (%)	
			Limit	Measured
22	SW	95	6.0	1.1895
23	SW	95	6.0	1.9665
24	SW	95	6.0	1.6080

- (1) Results for the remaining 'as received' samples are covered in BSI Test Report number 3220780 for the BSI COVID-19 filtering face piece technical specification testing.
- (2) Not a design feature of this product.

Test Results. (Continued)

CLAUSE	REQUIREMENTS	ASSESSMENT
--------	--------------	------------

7.9.2 Penetration of filter material (continued)

Table D: Clause 8.11. Exposure test Sodium Chloride.

	Sample 28 MS TC	Sample 29 MS TC	Sample 30 MS TC
Flow through filter	95 l/min		
Elapsed time (minutes)	Measured penetration % (Maximum permitted penetration 6.0 %)		
5	0.239798 (1)	0.100650 (1)	0.149081 (1)
10	0.192890	0.079177	0.121274
15	0.141387	0.065270	0.096979
20	0.090230	0.052679	0.076271
25	0.056086	0.041193	0.054319
30	0.033608	0.032297	0.038793
Result	Pass	Pass	Pass

- (1) The reading at which 5 subsequent sampling intervals showed a declining filter penetration. The testing was terminated without the 120mg exposure limit being reached, as permitted by BS EN 13274-7.

Test Results. (Continued)

CLAUSE	REQUIREMENTS	ASSESSMENT
--------	--------------	------------

7.9.2 Penetration of filter material (continued)

Table E: Clause 8.11 Paraffin oil exposure test.

	Sample 25 MS TC	Sample 26 MS TC	Sample 27 MS TC
Flow through filter	95 l/min		
Elapsed time (minutes)	Measured penetration % (Maximum permitted penetration 6.0 %)		
3	2.1110	1.5950	1.9965
5	2.2125	1.6255	2.0845
10	2.4525	1.9880	2.3595
15	2.5900	1.9280	2.4440
20	2.8495	1.9610	2.5800
25	3.0625	2.0000	2.6650
30	3.2990	2.1675	2.7670
35	3.2725	2.2115	2.9130
40	3.4220	2.2705	3.0045
45	3.6010	2.3765	3.0950
50	3.6315	2.3965	3.1885
55	3.7715	2.4610	3.2285
60	3.8520	2.5240	3.3385
(1)	4.0125	2.5060	3.3755
Result	Pass	Pass	Pass

(1) A loading of 120 mg was achieved after a period of 63 minutes, 10 seconds had elapsed.

Test Results. (Continued)

CLAUSE	REQUIREMENTS	ASSESSMENT															
7.10	<p>Compatibility with skin</p> <p>Materials that may come into contact with the wearer's skin shall not be known to be likely to cause irritation or any other adverse effect to health.</p> <p>Testing shall be done in accordance with 8.4 and 8.5.</p>	Pass															
7.11	<p>Flammability</p> <p>The material used shall not present a danger for the wearer and shall not be of a highly flammable nature.</p> <p>When tested, the particle filtering half mask shall not burn or not continue to burn for more than 5 seconds after removal from the flame.</p> <p>The particle filtering half mask does not have to be usable after the test.</p> <p>Testing shall be done in accordance with 8.6.</p> <p>Table F: Clause 8.6 – Flammability.</p> <table border="1"> <thead> <tr> <th>Sample</th> <th>Area exposed</th> <th>Comments</th> </tr> </thead> <tbody> <tr> <td>34 AR</td> <td>Filter material, welding.</td> <td>Did not ignite.</td> </tr> <tr> <td>35 AR</td> <td>Earloop, vertical welding.</td> <td>Did not ignite.</td> </tr> <tr> <td>36 TC</td> <td>Filter material, welding.</td> <td>Did not ignite.</td> </tr> <tr> <td>37 TC</td> <td>Earloop, vertical welding.</td> <td>Did not ignite.</td> </tr> </tbody> </table>	Sample	Area exposed	Comments	34 AR	Filter material, welding.	Did not ignite.	35 AR	Earloop, vertical welding.	Did not ignite.	36 TC	Filter material, welding.	Did not ignite.	37 TC	Earloop, vertical welding.	Did not ignite.	Pass See Table F
Sample	Area exposed	Comments															
34 AR	Filter material, welding.	Did not ignite.															
35 AR	Earloop, vertical welding.	Did not ignite.															
36 TC	Filter material, welding.	Did not ignite.															
37 TC	Earloop, vertical welding.	Did not ignite.															
7.13	<p>Head harness</p> <p>The head harness shall be designed so that the particle filtering half mask can be donned and removed easily.</p> <p>The head harness shall be adjustable or self-adjusting and shall be sufficiently robust to hold the particle filtering half mask firmly in position and be capable of maintaining total inward leakage requirements for the device.</p> <p>Testing shall be done in accordance with 8.4 and 8.5.</p>	Pass															
7.14	<p>Field of vision</p> <p>The field of vision is acceptable if determined so in practical performance tests.</p> <p>Testing shall be done in accordance with 8.4.</p>	Pass															

Test Results. (Continued)

CLAUSE	REQUIREMENTS	ASSESSMENT
--------	--------------	------------

7.16 Breathing resistance

The breathing resistances apply to valved and valveless particle filtering half masks and shall meet the requirements of Table 2.

Testing shall be done in accordance with 8.9.

A total of 9 valveless particle filtering half masks shall be tested:

3 as received, 3 after temperature conditioning in accordance with 8.3.2 and 3 after the test for simulated wearing in accordance with 8.3.1.

Pass* (1) (2)
See Tables G, H and I

Testing shall be done in accordance with 8.9.

A total of 12 valved particle filtering half masks shall be tested: 3 as received, 3 after temperature conditioning in accordance with 8.3.2, 3 after the test for simulated wearing in accordance with 8.3.1, and 3 after the flow conditioning in accordance with 8.3.4.

N/A (3)

Testing shall be done in accordance with 8.9.

Table G: Clause 8.9 – Breathing resistance. Inhalation resistance at a continuous flow.

Sample	Pre-test condition	Flow (l/min)	Limit (mbar)	Measured (mbar)
16	SW	30	0.7	0.54
17	SW	30	0.7	0.50
18	SW	30	0.7	0.53
31	TC	30	0.7	0.48
32	TC	30	0.7	0.47
33	TC	30	0.7	0.46

Table H: Clause 8.9 – Breathing resistance. Inhalation resistance at a continuous flow.

Sample	Pre-test condition	Flow (l/min)	Limit (mbar)	Measured (mbar)
16	SW	95	2.4	1.89
17	SW	95	2.4	1.87
18	SW	95	2.4	1.89
31	TC	95	2.4	1.79
32	TC	95	2.4	1.79
33	TC	95	2.4	1.72

- (1) Results for the remaining 'as received' samples are covered in BSI Test Report number 3220780 for the BSI COVID-19 filtering face piece technical specification testing.
- (2) Results for exhalation resistance are within the uncertainty of measurement, but compliance is more probable than non-compliance.
- (3) Not a design feature of this product.

Test Results. (Continued)

CLAUSE	REQUIREMENTS	ASSESSMENT
--------	--------------	------------

7.16 Breathing resistance (continued)

Table I: Clause 8.9 – Breathing resistance. Exhalation resistance at a continuous flow, measured in five orientations with the highest value recorded.

Sample	Pre-test condition	Flow (l/min)	Limit (mbar)	Measured (mbar)
16	SW	160	3.0	2.87
17	SW	160	3.0	2.96
18	SW	160	3.0	2.95
31	TC	160	3.0	2.89
32	TC	160	3.0	2.84
33	TC	160	3.0	2.79

Appendix A. – Test Panel Data

Test Candidate	Facial Dimensions (mm)					Gender
	Length of face	Width of face	Face depth	Width of mouth	Head Circumference	
JW1	116	126	122	48	570	Male
SI1	121	135	142	48	575	Male
LM2	110	148	125	47	567	Male
KH1	112	142	115	60	585	Male
CB1	117	147	130	57	566	Male

Note: All candidates were clean shaven

Product photographs.



Front view



Side view



Inside view

*** End of Report ***

Test Report No.: 244315789a 001
Client: SUNBEAM INTERNATIONAL GMBH
Contact Information: Schumanstr. 12, 52146 Würselen, Germany
 Contact Person: Edward Zhao

Sample Description As Declared:

No. Of Sample : 80 pcs
 Product Description : Personal Protective Respirator Mask
 Product Type : Single shift use only
 Material : -
 Colour : White
 Lot No./Batch Code : -
 Buyer Name : -
 Trademark : HYGISUN
 Type-identifying : HS0501A
 Claimed Classification : FFP2 NR
 Manufacturer : Hunan Dreaming Cloud E-Commerce Co., Ltd.
 Country of Origin : -
 Sales Destination (Country) : -
 Test Type : Full Test
 Test Specification : EN 149:2001 + A1:2009 Respiratory Protective Devices - Filtering Half Masks to Protect Against Particles - Requirements, Testing and Marking
 Other Information : -

Sample Obtaining Method: Sending by customer
Delivery Condition: Apparent good, samples tested as received
Sample Receiving date: 2021-03-04 & 2021-04-21
Testing Period: 2021-03-04 to 2021-04-01 & 2021-04-21 to 2021-04-27
Place of Testing: Textiles laboratory Shanghai

For and on behalf of
 TÜV Rheinland (Shanghai) Co., Ltd.



2021-04-30 Carmen Yan / Department Manager

Date Name/Position

*Sample information is provided by customer. Test result is drawn according to the kind and extent of tests performed.
 This test report relates to the above mentioned test sample. Without permission of the test center this test report is not permitted to be duplicated in extracts. This test report does not entitle to carry any safety mark on this or similar products.
 "Decision Rule" document announced in our website (<https://www.tuv.com/landingpage/en/qm-gcn/>) describes the statement of conformity and its rule of enforcement for test results are applicable throughout this test report.*

Test Report No.: 244315789a 001

Page 2 of 14

Summary of Test Results:

Clause	Item	Conclusion
7.3	Visual Inspection	P
7.4	Package	P
7.5	Material	P
7.6	Cleaning And Disinfection	N/A
7.7	Practical Performance	P
7.8	Finish Of Parts	P
7.9.1	Leakage	P
7.9.2	Penetration Of Filter Material	P
7.10	Compatibility With Skin	P
7.11	Flammability	P
7.12	Carbon Dioxide Content Of The Inhalation Air	P
7.13	Head Harness	P
7.14	Field Of Vision	P
7.15	Exhalation Valve(s)	N/A
7.16	Breathing Resistance	P
7.17	Clogging	N/A
7.18	Demountable Parts	N/A
10	Information To Be Supplied By The Manufacturer	P
9	Marking	P

Note: P = Pass F = Fail
 # = No Comment - = Did Not Perform
 N/R = Not Request N/A = Not Applicable

Material List:

Material No.	Material	Color	Location	Remark
M001	Whole Product	White	Personal Protective Respirator Mask	Received on 2021.03.04
M001'	Whole Product	White	Personal Protective Respirator Mask	Received on 2021.04.21

Test Report No.: 244315789a 001

Page 3 of 14

Visual Inspection

Test Method: EN 149:2001+A1:2009 Clause 8.2

Clause	Item	M001
7.3	The visual inspection shall also include the marking and the information supplied by the manufacturer.	Pass
7.4	Particle filtering half masks shall be offered for sale packaged in such a way that they are protected against mechanical damage and contamination before use.	Pass
7.5	Materials used shall be suitable to withstand handling and wear over the period for which the particle filtering half mask is designed to be used.	Pass
	After undergoing the conditioning described in 8.3.1 none of the particle filtering half masks shall have suffered mechanical failure of the face piece or straps.	Pass
	When conditioned in accordance with 8.3.1 and 8.3.2 the particle filtering half mask shall not collapse.	Pass
	Any material from the filter media released by the air flow through the filter shall not constitute a hazard or nuisance for the wearer.	Pass
7.8	Parts of the device likely to come into contact with the wearer shall have no sharp edges or burrs	Pass
7.18	All demountable parts (if fitted) shall be readily connected and secured, where possible by hand.	N/A

Remark:

N/A: Due to no relevant information/material

N/R: Due to not request

Test Report No.: 244315789a 001

Page 4 of 14

Practical Performance

Test Method: EN 149:2001+A1:2009 Clause 8.4 & 8.5

Clause	Item	M001
7.7	Wearing	Pass
7.7	Walking test	Pass
7.7	Work simulation test	Pass
7.10	Materials that may come into contact with the wearer's skin shall not be known to be likely to cause irritation or any other adverse effect to health	Pass
7.13	The head harness shall be designed so that the particle filtering half mask can be donned and removed easily. The head harness shall be adjustable or self-adjusting and shall be sufficiently robust to hold the particle filtering half mask firmly in position and be capable of maintaining total inward leakage requirements for the device	Pass
7.14	The field of vision is acceptable if determined so in practical performance tests	Pass

Remark:

N/A: Due to no relevant information/material

N/R: Due to not request

Test Report No.: 244315789a 001

Page 5 of 14

Clause 7.9.1: Leakage

Test Method : EN 149:2001+A1:2009 Clause 8.5

Requirement : FFP2 :

 At least 46 out of the 50 individual exercise results for total inward leakage \leq 11%

 At least 8 out of the 10 individual wearer arithmetic means for the total inward leakage \leq 8%

M001									
Condition	Specimen No.	Subject	Leakage (%)					Walk	Mean
			Walk	Head Side/Side	Head Up/Down	Talk			
As received	1	BM	4.927	7.304	9.711	5.581	2.803	6.065	
	2	ACH	3.824	6.874	8.145	8.664	5.217	6.545	
	3	ML	4.128	6.229	8.225	7.422	3.877	5.976	
	4	LLC	3.397	6.785	8.199	6.357	4.012	5.734	
	5	DG	3.981	6.932	8.902	7.559	4.331	6.341	
After conditioning	6	SG	4.104	5.181	10.648	7.685	3.493	6.222	
	7	YL	6.247	5.487	8.375	8.247	6.027	6.877	
	8	KQ	5.525	6.028	9.084	8.122	5.021	6.756	
	9	KXH	6.001	6.439	9.119	8.074	5.387	7.004	
	10	YY	5.743	6.009	8.911	7.936	5.111	6.742	
Conclusion		Pass							

Facial Dimension Of Subject (mm)											
Subject	BM	ACH	ML	LLC	DG	SG	YL	KQ	KXH	YY	LL
Face length	135	127	120	120	130	135	115	120	130	130	121
Face width	160	159	133	140	145	155	135	135	155	165	163
Face Depth	130	122	115	115	132	132	118	115	120	143	142
Mouth Width	52	55	52	50	50	55	48	50	52	50	45

Test Report No.: 244315789a 001

Page 6 of 14

Clause 7.9.2: Penetration Of Filter Material

Test method : EN 149:2001+A1:2009 Clause 8.11

Requirement : FFP2: ≤6%

M001			
Aerosol	Condition	Specimen No.	Penetration (%)
Sodium chloride Penetration	As received	1	0.048
	As received	2	0.223
	As received	3	0.226
	Simulated wearing treatment	4	0.568
	Simulated wearing treatment	5	0.483
	Simulated wearing treatment	6	0.439
	Mechanical strength + Temperature conditioned @ Exposure test of 120mg	7	0.322
	Mechanical strength + Temperature conditioned @ Exposure test of 120mg	8	0.282
	Mechanical strength + Temperature conditioned @ Exposure test of 120mg	9	0.289
Paraffin oil Penetration	As received	10	0.566
	As received	11	0.536
	As received	12	0.521
	Simulated wearing treatment	13	0.586
	Simulated wearing treatment	14	0.623
	Simulated wearing treatment	15	0.637
	Mechanical strength + Temperature conditioned @ Exposure test of 120mg	16	0.984
	Mechanical strength + Temperature conditioned @ Exposure test of 120mg	17	2.392
	Mechanical strength + Temperature conditioned @ Exposure test of 120mg	18	1.664
Conclusion	Pass		

Test Report No.: 244315789a 001

Page 7 of 14

Clause 7.11: Flammability

Test method : EN 149:2001+A1:2009 Clause 8.6

Requirement : ≤5s

M001			
Item	Condition	Specimen No.	Test results
Afterflame time (s)	As received	1	DNI
	As received	2	DNI
	After conditioning	3	DNI
	After conditioning	4	DNI
Conclusion		Pass	

Remark:

DNI-Do not ignite

Test Report No.: 244315789a 001

Page 8 of 14

Clause 7.12: Carbon Dioxide Content Of The Inhalation Air

Test Method : EN 149:2001+A1:2009 Clause 8.7

Requirement : ≤1%

M001			
Item	Condition	Test results	
Content (%)	As received	Specimen 1	0.58
	As received	Specimen 2	0.59
	As received	Specimen 3	0.61
	As received	Mean	0.60
Conclusion		Pass	

Test Report No.: 244315789a 001

Page 9 of 14

Clause 7.16: Breathing Resistance

Test Method : EN 149:2001+A1:2009 Clause 8.9

Requirement : FFP2:

Inhalation: 30l/min: ≤0.7mbar

Inhalation: 95l/min: ≤2.4mbar

Exhalation: 160l/min: ≤3.0mbar

M001'																
Flow rate (l/min)		Resistance (mbar)														
As received		Specimen 1					Specimen 2					Specimen 3				
		A	B	C	D	E	A	B	C	D	E	A	B	C	D	E
Inhalation	30	0.4	0.4	0.4	0.4	0.4	0.5	0.5	0.5	0.5	0.5	0.4	0.4	0.4	0.4	0.4
	95	1.3	1.3	1.3	1.3	1.3	1.4	1.4	1.4	1.4	1.4	1.4	1.4	1.4	1.4	1.4
Exhalation	160	2.0	2.0	2.0	2.0	2.0	2.2	2.2	2.2	2.2	2.2	2.2	2.2	2.2	2.2	2.2
Simulated wearing treatment		Specimen 4					Specimen 5					Specimen 6				
		A	B	C	D	E	A	B	C	D	E	A	B	C	D	E
Inhalation	30	0.5	0.5	0.5	0.5	0.5	0.5	0.5	0.5	0.5	0.5	0.5	0.5	0.5	0.5	0.5
	95	1.5	1.5	1.5	1.5	1.5	1.4	1.4	1.4	1.4	1.4	1.5	1.5	1.5	1.5	1.5
Exhalation	160	2.4	2.4	2.4	2.4	2.4	2.3	2.3	2.3	2.3	2.3	2.3	2.3	2.3	2.3	2.3
Temperature conditioned		Specimen 7					Specimen 8					Specimen 9				
		A	B	C	D	E	A	B	C	D	E	A	B	C	D	E
Inhalation	30	0.4	0.4	0.4	0.4	0.4	0.5	0.5	0.5	0.5	0.5	0.5	0.5	0.5	0.5	0.5
	95	1.4	1.4	1.4	1.4	1.4	1.5	1.5	1.5	1.5	1.5	1.5	1.5	1.5	1.5	1.5
Exhalation	160	2.3	2.3	2.3	2.3	2.3	2.4	2.4	2.4	2.4	2.4	2.2	2.2	2.2	2.2	2.2
Conclusion		Pass														

Remark : A: facing directly ahead;
 B: facing vertically upwards;
 C: facing vertically downwards;
 D: lying on the left side;
 E: lying on the right side

Test Report No.: 244315789a 001

Page 10 of 14

Marking

Test Method: EN 149:2001+A1:2009 Clause 9

M001	
9.1 Packaging	
The following information shall be clearly and durably marked on the smallest commercially available packaging or legible through it if the packaging is transparent.	
9.1.1 The name, trademark or other means of identification of the manufacturer or supplier.	Present
9.1.2 Type-identifying marking.	Present
9.1.3 Classification The appropriate class (FFP1, FFP2 or FFP3) followed by a single space and then: "NR" if the particle filtering half mask is limited to single shift use only. Example: FFP3 NR, or "R" if the particle filtering half mask is re-usable. Example: FFP2 R D.	Present
9.1.4 The number and year of publication of this European Standard.	Present
9.1.5 At least the year of end of shelf life. The end of shelf life may be informed by a pictogram as shown in Figure 12a, where yyyy/mm indicates the year and month.	Present
9.1.6 The sentence 'see information supplied by the manufacturer', at least in the official language(s) of the country of destination, or by using the pictogram as shown in Figure 12b.	Present
9.1.7 The manufacturer's recommended conditions of storage (at least the temperature and humidity) or equivalent pictogram, as shown in Figures 12c and 12d.	Present
9.1.8 The packaging of those particle filtering half masks passing the dolomite clogging test shall be additionally marked with the letter "D". ID This letter shall follow the classification marking preceded by a single space.	N/A
9.2 Particle filtering half mask	
Particle filtering half masks complying with this European Standard shall be clearly and durably marked with the following:	
9.2.1 The name, trademark or other means of identification of the manufacturer or supplier.	Present
9.2.2 Type-identifying marking.	Present
9.2.3 The number and year of publication of this European Standard.	Present
9.2.4 Classification The appropriate class (FFP1, FFP2 or FFP3) followed by a single space and then: "NR" if the particle filtering half mask is limited to single shift use only. Example: FFP3 NR, or "R" if the particle filtering half mask is re-usable. Example: FFP2 R D.	Present
9.2.5 If appropriate the letter D (dolomite) in accordance with clogging performance. This letter shall follow the classification marking preceded by a single space.	N/A
9.2.6 Sub-assemblies and components with considerable bearing on safety shall be marked so that they can be identified.	N/A

Test Report No.: 244315789a 001

Page 11 of 14

Remark:

1. The evaluation is based on artwork.
2. N/A: Not applicable

Test Report No.: 244315789a 001

Page 12 of 14

Information To Be Supplied By The Manufacturer

Test Method: EN 149:2001+A1:2009 Clause 10

M001	
10.1 Information supplied by the manufacturer shall accompany every smallest commercial available package	Present
10.2 Information supplied by the manufacturer shall be at least in the official language(s) of the country of destination	Present
10.3 The information supplied by the manufacturer shall contain all information necessary for trained and qualified persons on	
- application/limitations	Present
- the meaning of any colour coding	N/A
- checks prior to use	Present
- donning, fitting	Present
- use	Present
- maintenance (e.g. cleaning, disinfecting), if applicable	N/A
- storage	Present
- the meaning of any symbols/pictograms used	Present
of the equipment	
10.4 The information shall be clear and comprehensible. If helpful, illustrations, part numbers, marking shall be added	Present
10.5 Warning shall be given against problems likely to be encountered, for example:	
- fit of particle filtering half mask (check prior to use)	Present
- it is unlikely that the requirements for leakage will be achieved if facial hair passes under the face seal	Present
- air quality (contaminants, oxygen deficiency)	Present
- use of equipment in explosive atmosphere	Present
10.6 The information shall provide recommendations as to when the particle filtering half mask shall be discarded	Present
10.7 For devices marked "NR", a warning shall be given that the particle filtering half mask shall not be used for more than one shift	Present



Remark:

1. The evaluation is based on artwork.
2. N/A: Not applicable

Test Report No.: 244315789a 001

Page 13 of 14


Photo(s):

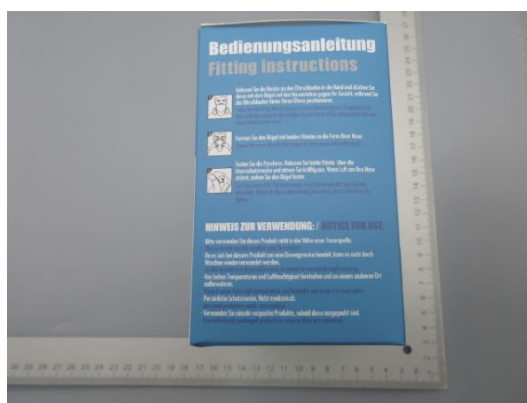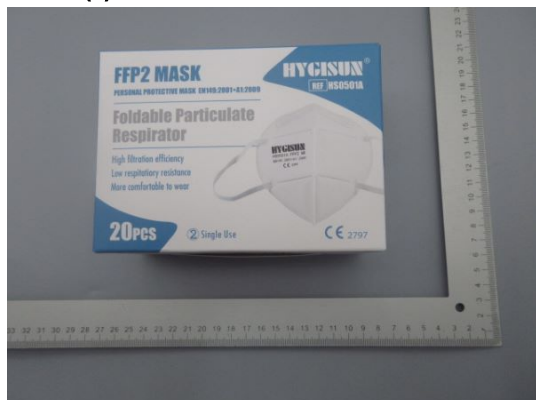

Test Report No.: 244315789a 001

Page 14 of 14

Photo(s):

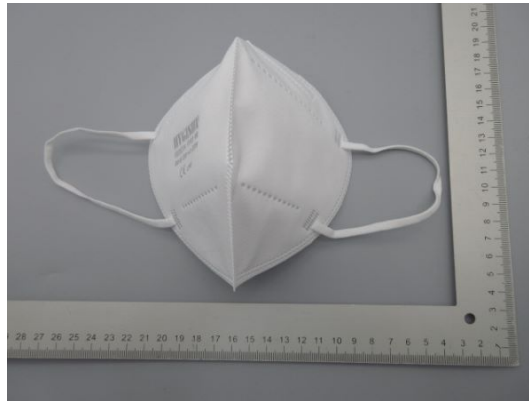

- END -

